






+



If your inhaler runs out, simply detach the smart sensor from the old one and attach it to the new inhaler.


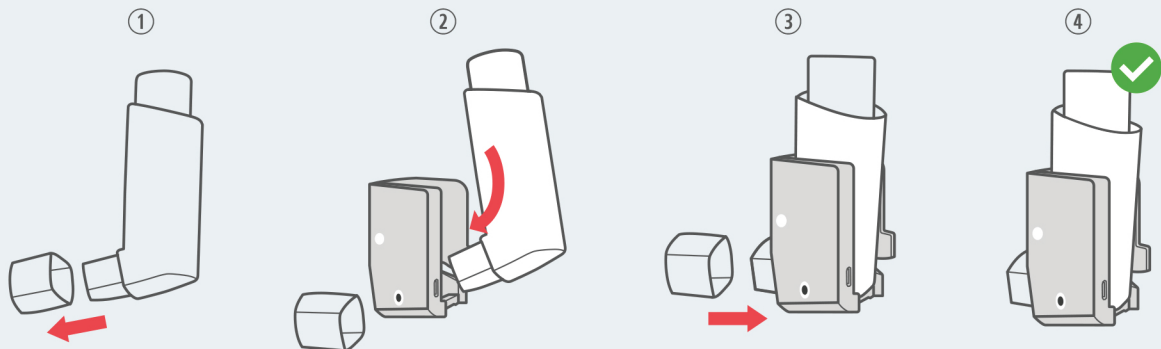


+

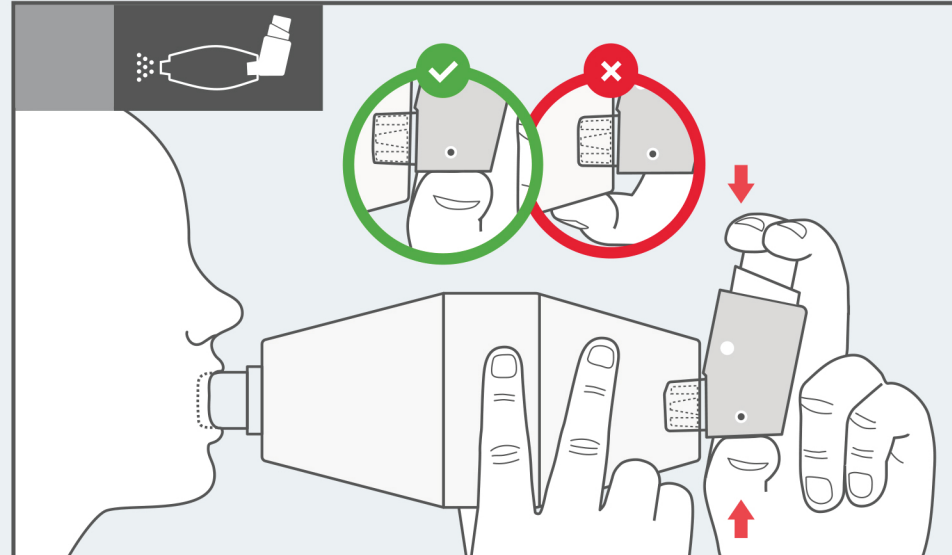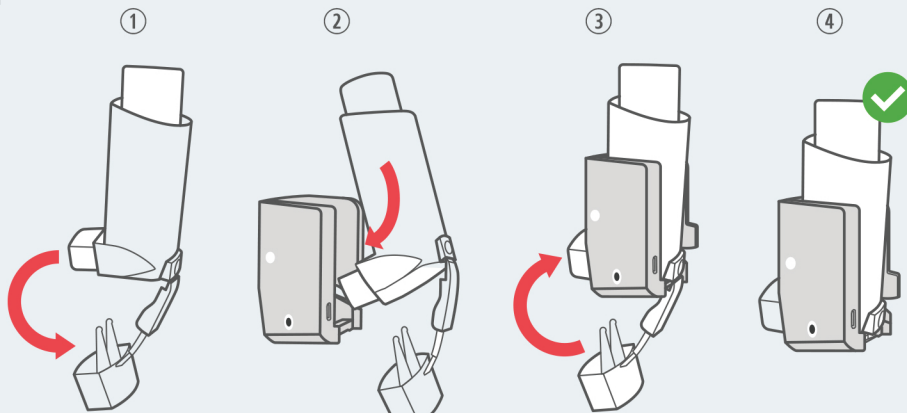

Digital Smart Inhaler Asthma Management in Children and Young People

asthma.medicalstudy.co.uk
01234 567 890
support@medicalstudy.co.uk

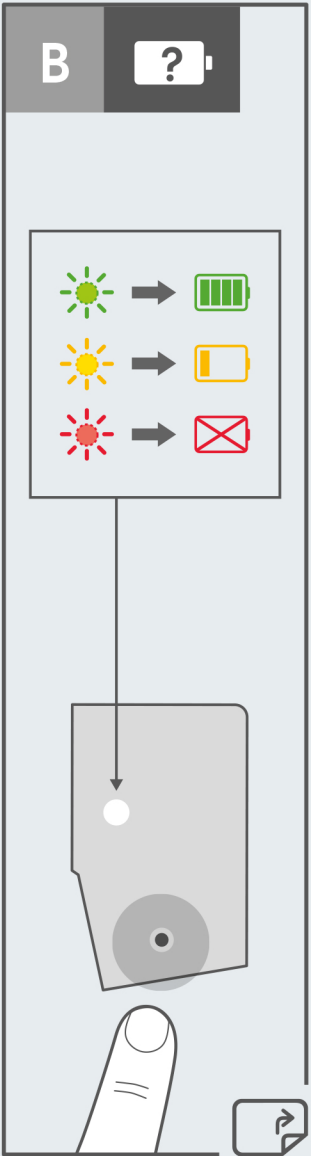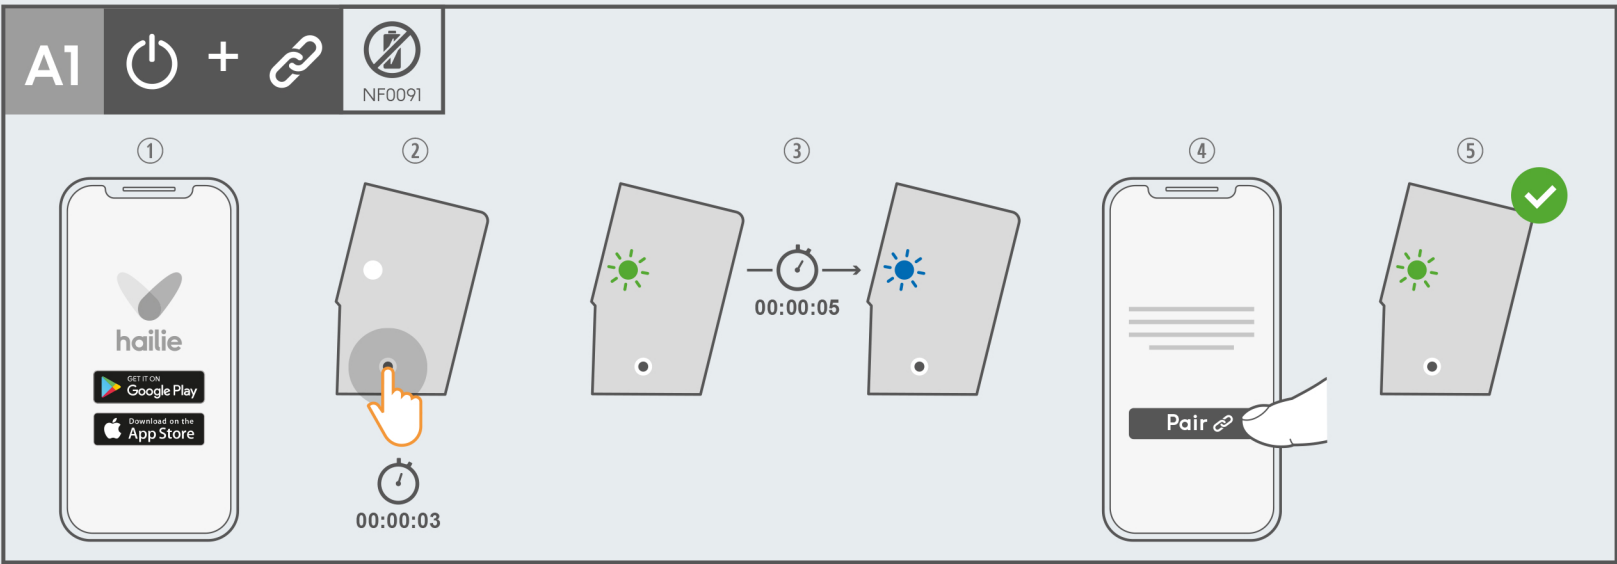

 NF0090  NF0091

EC REP

Emergo Europe
Westervoortedijk 60
6827 AT, Arnhem
The Netherlands

CE EU 2017/745,
2014/53/EU, 2011/65/EU